
An ke lin Particle Filtering Half Mask

1. Basic Information (Page 1)
2. Pictures (Page 1-3)
3. Certificats (Page 4-7)
4. Test reports (Page 8-17)
5. EU Declaration of Conformity (Page 18)

1. Basic Information

Brand: An ke lin

Model: Filtering Half Mask, KZ888E

CE standard: EN 149:2001+A1:2009

Classifications: FFP2 NR

Material: Non-woven Fabric, Melt-blown Fabric

Design: Ear loops with head harness clip, no valves, internal metal nose clip

Size: 16cm*10.7cm

Expiration date: 2 years

Packaging:

25pcs per box, 32 boxes per carton, 800 pcs per carton

Box Size: 19.5*15*8.5cm

Carton Size: 62*41*37cm

Gross Weight: 10.3 kg

2. Pictures



合格证/Inspection Certificate

产品名称 (Product) 颗粒物过滤口罩
Particle Filtering Half Mask
产品型号 (Model) KZ888E
原材料 (Raw Material) 无纺布/Non-woven Fabric50%+熔喷布
/Melt-blown Fabric50%
执行标准 (Product Standard) EN149:2001+A1:2009 FFP2 NR
数量 (Quantity) 1只/Pcs
生产批号 (LOT) 2010416
生产日期 (MFG) 20201102
贮存期限 (EXP) 2年/Years
检验员 (Inspectors) _____



河南省安克林滤业有限公司
Henan Akilly Filter Engineering Co.,Ltd

地址：河南省长垣市南蒲区宏力大道南段
Add:The South Section Of Hongli Road,Nanpu District,
Changyuan City,Henan Province.
电话/Tel: 0373-8722618 <http://www.hnsakilly.com>

非医用/Non-Medical MADE IN CHINA



Module B EU Type-Examination Certificate

For the requirements of PPE Regulation 2016/425

Certificate No.: CE-PC-200508-351-01-9A

| | |
|----------------------------|---|
| Certificate holder: | Henan Akily Filter Engineering Co., Ltd. The South Section of Hongli Road, Nanpu District, Changyuan City, Henan Province, China |
| Product: | Particle Filtering Half Mask Detailed product description listed in the Annex |
| Model(s): | KZ888E |
| Standard(s): | EN 149:2001+A1:2009 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking |
| Issue date: | 2020-07-03 |
| Revision date: | 2020-07-03 |
| Expiry date: | 2021-07-02 |

The product(s) on this certificate and the Technical File have been assessed and found to be in conformance with the applicable Essential Health and Safety Requirements in Annex II of the PPE regulation 2016/425.

Any changes to the design, manufacturing location or manufacture of the PPE product certified here must be advised to CCQS Certification Services Limited for review.

CE marking shall not be applied until the requirements of all the PPE Regulation 2016/425 and relevant EN Harmonised standards and/or Technical specifications have been met.

If the certified product is Category III then this certificate is only valid if used in conjunction with Conformity Assessment against Module C2 or Module D.

This certificate remains the property of CCQS and maybe withdrawn at any time if it is considered that the equipment is no longer in conformity with the requirements of the PPE Regulation 2016/425.



Approved by Ireland
Government
as a Notified Body
for CE Marking No.2834



Approved by:


Owen Brian, Director

CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15,
D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie
If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.

Page 1 of 2
(Fm 220-017, Rev.2)



Module B EU Type-Examination Certificate Annex

For the requirements of PPE Regulation 2016/425

Certificate No.: CE-PC-200508-351-01-9A

Applicable standards and specification:

EN 149:2001+A1:2009 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking

| Model reference | Product description |
|-----------------|---|
| KZ888E | Folding filtering half mask fitted with ear loops with head harness clip, no valves, internal metal nose clip Classification: FFP2 NR Test report No.: 2020(D) - 0673 |

| Certificate Revision | Revision date | Revision details |
|----------------------|---------------|------------------|
| A | 2020-07-03 | Initial issue |



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie
If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.

Page 2 of 2
(Fm 220-017, Rev.2)



Certificate of Module C2 production monitoring for equipment within the scope of Personal Protective Equipment Regulation (EU) 2016/425 Category III

FPC Certificate No.: CE-PC-200508-351-FPC-A

| | |
|--|---|
| Certificate holder: | Henan Akly Filter Engineering Co., Ltd. The South Section of Hongli Road, Nanpu District, Changyuan City, Henan Province, China |
| Manufacturing Location: | The South Section of Hongli Road, Nanpu District, Changyuan City, Henan Province, China |
| The scope of the certification for: | The manufacture of respiratory protective device See annex for articles covered by this certificate |
| Validity from: | 2020-07-03 |
| Revision date: | 2020-07-03 |
| To: | 2021-07-02 |

CCQS Certification Services Limited in its role as a Notified Body for PPE Regulation, is monitoring that the manufacturer is producing PPE in conformity with the type described in the EU type-examination certificate and associated technical file and which satisfies the Essential Health and Safety Requirements of the Regulation. The equipment covered by this certificate is listed in the accompanying schedule. This certificate is not complete and has no validity without the accompanying schedule and revision index. The manufacturer is hereby authorized to affix our Notified Body number, 2834, to each item of PPE mentioned in the schedule which accompanies this certificate whilst this certificate remains valid. This certificate and the accompanying schedule remain the property of CCQS and maybe withdrawn or revised at any time if CCQS considers that the equipment is no longer in conformity with the requirements of the Regulation.



Approved by Ireland
Government
as a Notified Body
for CE Marking No.2834



Approved by:

Owen Bian, Director



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15,
D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie

If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.

Page 1 of 2
(Fm 220-015, Rev.2)



Schedule of Module C2 production monitoring for equipment within the scope of Personal Protective Equipment Regulation (EU) 2016/425 Category III

Schedule to CCQS FPC Certificate No.: CE-PC-200508-351-FPC-A

| Product reference and description | | Reference standard |
|-----------------------------------|---------------|---------------------|
| Particle Filtering Half Mask | Model: KZ888E | EN 149:2001+A1:2009 |

| Certificate Revision | Revision date | Revision details |
|----------------------|---------------|------------------|
| A | 2020-07-03 | Initial issue |

This schedule has no validity without the accompanying certificate.

This schedule and the accompanying certificate remain the property of CCQS and maybe withdrawn or revised at any time if CCQS considers that the equipment is no longer in conformity with the requirements of the Regulation.



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie
If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.



Page 2 of 2
(Fm 220-015, Rev.2)

4. Test reports



中国认可
国际互认
检测
TESTING
CNAS L1499

National Quality Supervision and Testing Center for Personal
Protective Equipment (Beijing)
(Testing Laboratory for Labour Protection Products of Beijing
Municipal Institute for Labour Protection)

No.55 Taoranting Street, Xicheng District, Beijing, China.
Phone: +86 10 63519250 +86 10 63520770 +86 10 83530311
Fax: +86 10 63519250 +86 10 63520770

The Testing Center is accredited for compliance with ISO/IEC 17025.

The results of tests, calibrations and/or measurements included in this document are traceable to Chinese/national standards.

CNAS is a signatory to the ILAC mutual recognition arrangement for the mutual recognition of the equivalence of testing, calibration and inspection reports.

TEST REPORT

Particulate respirator-half facepiece

EN 149: 2001 +A1: 2009 Respiratory protective devices — Filtering half masks to protect against particles —
Requirements, testing, marking

Product: Particle filtering half mask
Report No: 2020 (D) – 0673
Client: Henan Akly Filter Engineering Co., Ltd.
Model (s): KZ888E
Date(s) of tests: 2020.05.11-2020.06.01

DESCRIPTION OF SAMPLES

| General Information | Classification | Main Components |
|--|--|--------------------|
| Manufacturer Manufacturer Address | FFP2 NR Henan Akly Filter Engineering Co., Ltd. The South Section of Hongli Road, Nanpu District, Changyuan City, Henan Province | White folding mask |

Signed:

陈倬为 Chen Zhuowei
Authorized Signatory, Lab Director

Issued: 2020.6.1

Page 1 of 10



This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动防护用品质量监督检验中心(北京)

Conditions:

The test results presented in this report relate to the samples tested only.

This report may be reproduced and distributed to your clients, provided that it is reproduced and distributed in full.

The authenticity of this test report and its contents can be verified by contacting the laboratory.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动防护用品质量监督检验中心(北京)

Test Results

| | | | | | | | |
|--|-------------------------------|----------------------------|------|------|------|------|-------------------------|
| <p>7.3 Visual inspection The visual inspection shall include the marking and information supplied by the manufacturer. Note1: As requested by the client, marking and information supplied by the manufacturer was not inspected.</p> | Not tested¹ | | | | | | |
| <p>7.4 Package Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use. Note2: In accordance with the requirement.</p> | Pass² | | | | | | |
| <p>7.5 Material Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used. Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer. After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps. When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse. Note3: No mechanical failure after undergoing the conditioning described in 8.3.1. No collapse when conditioned in accordance with 8.3.1 and 8.3.2.</p> | Pass³ | | | | | | |
| <p>7.6 Cleaning and disinfecting If the particle filtering half mask is designed to be re-usable, the materials used shall withstand the cleaning and disinfecting agents and procedures to be specified by the manufacturer. Note4: Single shift use only.</p> | N/A⁴ | | | | | | |
| <p>7.7 Practical performance The particle filtering half mask shall undergo practical performance tests under realistic conditions. Note5: No imperfections.</p> | Pass⁵ | | | | | | |
| <p>7.8 Finish of parts Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs. Note6: No sharp edges or burrs.</p> | Pass⁶ | | | | | | |
| <p>7.9.1 Total inward leakage For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than 22% for FFP1, 8% for FFP2, 2% for FFP3 Note7: FFP2 respirator. Test results are shown in Annex A Table 7.9.1-A&B.</p> | Pass⁷ | | | | | | |
| <p>7.9.2 Penetration of filter material The penetration of the filter of the particle filtering half mask shall meet the requirements of Table 1. <table border="0" style="margin-left: 40px; width: 80%;"> <tr> <td style="width: 50%;">Sodium chloride test 95 l/min</td> <td style="width: 50%;">Paraffin oil test 95 l/min</td> </tr> <tr> <td>FFP1</td> <td>FFP1</td> </tr> <tr> <td style="text-align: center;">≤20%</td> <td style="text-align: center;">≤20%</td> </tr> </table> </p> | Sodium chloride test 95 l/min | Paraffin oil test 95 l/min | FFP1 | FFP1 | ≤20% | ≤20% | Pass⁸ |
| Sodium chloride test 95 l/min | Paraffin oil test 95 l/min | | | | | | |
| FFP1 | FFP1 | | | | | | |
| ≤20% | ≤20% | | | | | | |
| <p>This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.</p> | | | | | | | |

| | | |
|------|-----|-----|
| FFP2 | ≤6% | ≤6% |
| FFP3 | ≤1% | ≤1% |

Note8: FFP2 respirator. Test results are shown in Annex A Table 7.9.2.

7.10 Compatibility with skin

Pass⁹

Materials that may come into contact with the wearer’s skin shall not be known to be likely to cause irritation or any other adverse effect to health.

Note9: No irritation or any other adverse effect to health.

7.11 Flammability

Pass¹⁰

When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame.

Note10: Test results are shown in Annex A Table 7.11.

7.12 Carbon dioxide content of the inhalation air

Pass¹¹

The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)

Note11: Test results are shown in Annex A Table 7.12.

7.13 Head harness

Pass¹²

The head harness shall be designed so that the particle filtering half mask can be donned and removed easily. The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.

Note12: Head harness can be donned and removed easily, adjustable or self-adjusting and have sufficiently robust to hold the particle filtering half mask firmly.

7.14 Field of vision

Pass¹³

The field of vision is acceptable if determined so in practical performance tests.

Note13: Pass the practical performance tests.

7.15 Exhalation valve

N/A¹⁴

A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations.

If an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device that may be necessary for the particle filtering half mask to comply with 7.9.

Exhalation valve(s), if fitted, shall continue to operate correctly after a continuous exhalation flow of 300 l/min over a period of 30 s.

When the exhalation valve housing is attached to the faceblank, it shall withstand axially a tensile force of 10 N applied for 10 s.

Note14: No exhalation valve.

7.16 Breathing resistance

Pass¹⁵

| Classification | Maximum permitted resistance (mbar) | | |
|----------------|-------------------------------------|----------|------------|
| | Inhalation | | Exhalation |
| | 30 l/min | 95 l/min | 160 l/min |
| FFP1 | 0.6 | 2.1 | 3.0 |
| FFP2 | 0.7 | 2.4 | 3.0 |
| FFP3 | 1.0 | 3.0 | 3.0 |

Note15: FFP2 respirator. Test results are shown in Annex A Table 7.16.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

7.17 Clogging

N/A¹⁶

7.17.2 Breathing resistance

Valved particle filtering half masks:

After clogging the inhalation resistances shall not exceed:

FFP1: 4 mbar, FFP2: 5 mbar, FFP3: 7 mbar at 95L/min continuous flow

The exhalation resistance shall not exceed 3 mbar at 160 L/min continuous flow

Valveless particle filtering half masks

After clogging the inhalation and exhalation resistances shall not exceed:

FFP1: 3 mbar, FFP2: 4 mbar, FFP3: 5 mbar at 95L/min continuous flow

7.17.3 Penetration of filter material

| | Sodium chloride test 95 l/min | Paraffin oil test 95 l/min |
|------|-------------------------------|----------------------------|
| FFP1 | ≤20% | ≤20% |
| FFP2 | ≤6% | ≤6% |
| FFP3 | ≤1% | ≤1% |

Note16: Single shift use only.

7.18 Demountable parts

Pass¹⁷

All demountable parts (if fitted) shall be readily connected and secured, where possible by hand

Note17: In accordance with the requirement.

9 Marking

Not tested

9.1 Packaging

The following information shall be clearly and durably marked on the smallest commercially available packaging or legible through it if the packaging is transparent.

9.1.1 The name, trademark or other means of identification of the manufacturer or supplier.

9.1.2 Type-identifying marking.

9.1.3 Classification

The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable.

Example: FFP2 R D.

9.1.4 The number and year of publication of this European Standard.

9.1.5 At least the year of end of shelf life. The end of shelf life may be informed by a pictogram as shown in Figure 12a, where yyyy/mm indicates the year and month.

9.1.6 The sentence 'see information supplied by the manufacturer', at least in the official language(s) of the country of destination, or by using the pictogram as shown in Figure 12b.

9.1.7 The manufacturer's recommended conditions of storage (at least the temperature and humidity) or equivalent pictogram, as shown in Figures 12c and 12d.

9.1.8 The packaging of those particle filtering half masks passing the dolomite clogging test shall be additionally marked with the letter "D". This letter shall follow the classification marking preceded by a single space.

9.2 Particle filtering half mask

Particle filtering half masks complying with this European Standard shall be clearly and durably marked with the following:

9.2.1 The name, trademark or other means of identification of the manufacturer or supplier.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

9.2.2 Type-identifying marking.

9.2.3 The number and year of publication of this European Standard.

9.2.4 Classification

The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable. Example: FFP2 R D.

9.2.5 If appropriate the letter D (dolomite) in accordance with clogging performance. This letter shall follow the classification marking preceded by a single space

9.2.6 Sub-assemblies and components with considerable bearing on safety shall be marked so that they can be identified.

End of Test Results

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

國家勞動保護用品質量監督檢驗中心(北京)

Annex A: Summarization of Test Data**Table 7.9.1-A Inward leakage test data**

Test specification: EN 149-2001 Clause 8.5

| Subject | Sample No. | Condition | Walk(%) | Head Side/side(%) | Head up/down(%) | Talk(%) | Walk(%) | Mean(%) |
|--|------------|-----------|---------|-------------------|-----------------|---------|---------|---------|
| Yi | 1 | A.R. | 7.12 | 7.69 | 7.52 | 7.14 | 7.34 | 7.4 |
| Gong | 2 | A.R. | 7.22 | 7.71 | 7.66 | 7.24 | 7.41 | 7.4 |
| Yu | 3 | A.R. | 7.07 | 7.51 | 7.23 | 7.50 | 7.28 | 7.3 |
| Hu | 4 | A.R. | 8.84 | 8.97 | 9.23 | 8.84 | 9.22 | 9.0 |
| Xu | 5 | A.R. | 7.15 | 7.42 | 7.33 | 7.51 | 7.44 | 7.4 |
| Deng | 6 | T.C. | 7.27 | 7.42 | 7.65 | 7.28 | 7.43 | 7.4 |
| Zhang | 7 | T.C. | 6.39 | 6.79 | 6.81 | 6.60 | 6.55 | 6.6 |
| Liu | 8 | T.C. | 6.30 | 6.69 | 6.39 | 6.46 | 6.79 | 6.5 |
| Zhi | 9 | T.C. | 7.11 | 7.70 | 7.61 | 7.49 | 7.24 | 7.4 |
| Fang | 10 | T.C. | 8.04 | 8.51 | 8.36 | 8.32 | 8.49 | 8.3 |
| All <u>50</u> individual exercise results were not greater than <u>11</u> % <u>8</u> out of <u>10</u> individual wearer arithmetic means were not greater than <u>8</u> % | | | | | | | Pass | |

Table 7.9.1-B Facial dimension

| Subject | Face length | Face Width | Face Depth | Mouth Width |
|---------|-------------|------------|------------|-------------|
| Yi | 120 | 130 | 109 | 59 |
| Gong | 122 | 140 | 115 | 65 |
| Yu | 119 | 160 | 139 | 55 |
| Hu | 112 | 122 | 119 | 63 |
| Xu | 110 | 130 | 118 | 60 |
| Deng | 115 | 119 | 110 | 59 |
| Zhang | 112 | 123 | 113 | 55 |
| Liu | 103 | 130 | 100 | 50 |
| Zhi | 118 | 139 | 130 | 63 |
| Fang | 115 | 129 | 120 | 50 |
| Chen | 116 | 150 | 132 | 56 |
| Lv | 110 | 121 | 110 | 53 |

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动防护用品质量监督检验中心(北京)

Table -7.9.2 Penetration of filter material

Test specification: EN 149-2001 Clause 8.11

| Aerosol | Condition | Sample No. | Penetration (%) | Assessment |
|--|--|------------|-----------------|------------|
| Sodium chloride test | As received | 11 | 0.211 | Pass |
| | | 12 | 0.289 | |
| | | 13 | 0.342 | |
| | Simulated wearing treatment | 14 | 0.511 | |
| | | 15 | 0.638 | |
| | | 16 | 0.572 | |
| | Mechanical strength+ Temperature conditioned | 17 | 0.894 | |
| | | 18 | 0.962 | |
| | | 19 | 1.04 | |
| Paraffin oil test | As received | 20 | 2.71 | Pass |
| | | 21 | 2.96 | |
| | | 22 | 3.11 | |
| | Simulated wearing treatment | 23 | 3.09 | |
| | | 24 | 3.48 | |
| | | 25 | 3.51 | |
| | Mechanical strength+ Temperature conditioned | 26 | 4.04 | |
| | | 27 | 3.92 | |
| | | 28 | 4.61 | |
| Flow conditioning: Single filter: 95.0 L/min | | | | |

Table 7.11 Flammability

Test specification: EN 149-2001 Clause 8.6

| Condition | Sample No. | Result | Assessment |
|-------------------------|------------|--------------|------------|
| As received | 29 | Burn for 1 s | Pass |
| | 30 | Burn for 2 s | |
| Temperature conditioned | 31 | Burn for 2 s | |
| | 32 | Burn for 1 s | |

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

國家勞動保護用品質量監督檢驗中心(北京)

Table 7.12 Carbon dioxide content of the inhalation air

Test specification: EN 149-2001 Clause 8.7

| Condition | Sample No. | Result | Assessment |
|-------------|------------|--------|--------------------|
| As received | 33 | 0.44% | Mean value 0.4% |
| | 34 | 0.47% | |
| | 35 | 0.42% | |
| | | | Pass |

Table 7.16 Breathing resistance (mbar)

Test specification: EN 149-2001 Clause 8.9

| As received | Flow rate | | 36 | | | | | 37 | | | | | 38 | | | | |
|-----------------------------|------------|-----------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| | | | A | B | C | D | E | A | B | C | D | E | A | B | C | D | E |
| As received | Inhalation | 30 l/min | 0.4 | 0.5 | 0.6 | 0.5 | 0.5 | 0.4 | 0.6 | 0.6 | 0.5 | 0.4 | 0.4 | 0.5 | 0.5 | 0.5 | 0.4 |
| | | 95 l/min | 1.6 | 1.6 | 1.8 | 1.8 | 1.6 | 1.6 | 1.7 | 1.9 | 1.8 | 1.8 | 1.7 | 1.8 | 2.0 | 1.7 | 1.6 |
| | Exhalation | 160 l/min | 1.9 | 2.0 | 2.0 | 1.9 | 2.0 | 1.8 | 1.9 | 2.1 | 2.0 | 1.9 | 1.9 | 2.0 | 2.0 | 2.0 | 1.9 |
| Simulated wearing treatment | Flow rate | | 39 | | | | | 40 | | | | | 41 | | | | |
| | Inhalation | 30 l/min | 0.4 | 0.5 | 0.6 | 0.5 | 0.5 | 0.5 | 0.5 | 0.6 | 0.5 | 0.5 | 0.4 | 0.5 | 0.6 | 0.5 | 0.4 |
| | | 95 l/min | 1.7 | 1.8 | 2.0 | 1.8 | 1.7 | 1.6 | 1.9 | 2.0 | 1.8 | 1.8 | 1.7 | 1.9 | 1.9 | 1.8 | 1.8 |
| Exhalation | 160 l/min | 1.9 | 1.9 | 2.1 | 2.2 | 1.9 | 1.8 | 2.2 | 2.3 | 2.1 | 2.0 | 1.9 | 2.1 | 2.2 | 2.0 | 2.0 | |
| Temperature conditioned | Flow rate | | 42 | | | | | 43 | | | | | 44 | | | | |
| | Inhalation | 30 l/min | 0.4 | 0.5 | 0.6 | 0.5 | 0.4 | 0.4 | 0.5 | 0.6 | 0.5 | 0.4 | 0.5 | 0.5 | 0.6 | 0.5 | 0.4 |
| | | 95 l/min | 1.7 | 1.8 | 2.0 | 1.9 | 1.8 | 1.6 | 1.8 | 1.9 | 1.9 | 1.8 | 1.7 | 1.8 | 2.0 | 1.8 | 1.7 |
| Exhalation | 160 l/min | 1.9 | 2.0 | 2.2 | 2.2 | 2.0 | 1.8 | 1.9 | 2.2 | 2.1 | 1.9 | 2.0 | 2.1 | 2.2 | 2.0 | 2.0 | |
| Assessment | Pass | | | | | | | | | | | | | | | | |




A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side

End of Annex A

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动保护用品质量监督检验中心(北京)

ANNEX B PHOTOS OF SAMPLES

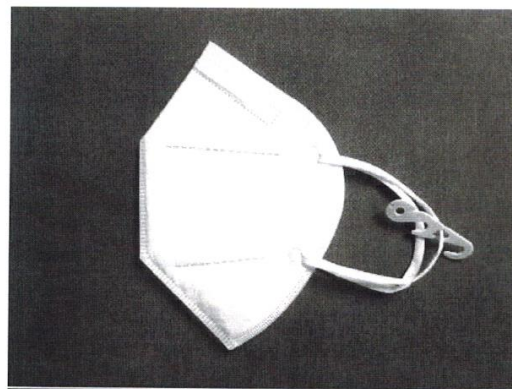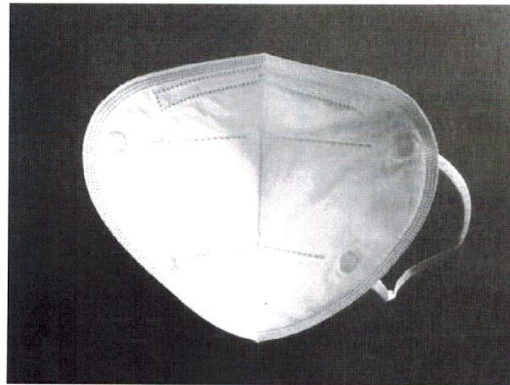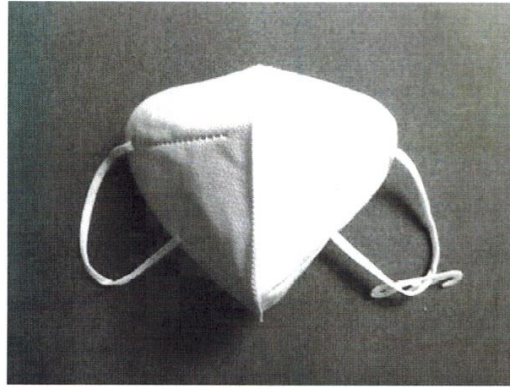

End of Annex B

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动保护用品质量监督检验中心(北京)

5. EU Declaration of Conformity

EU Declaration of Conformity

Annex IX PPE Regulation (EU) 2016/425

This EU Declaration of conformity refers to the following products

| 1 | Product Name | Model | Classification/Type | Batch No./Serial No./Identifier |
|---|------------------------------|--------|---------------------|---------------------------------|
| | Particle Filtering half mask | KZ888E | FFP2 NR | -- |

2. The Manufacturer's name and address is as follows:

| | |
|----------|---|
| Name: | Henan Akly Filter Engineering Co., Ltd |
| Address: | The South Section Of Hongli Road, Nanpu District, Changyuan City, Henan Province, China |


3. This Declaration of Conformity is issued under the sole responsibility of the Manufacturer.

4. Detailed description of the PPE to allow traceability/identification of the PPE.

Model: KZ888E

FFP2 NR

White folding half mask without valve

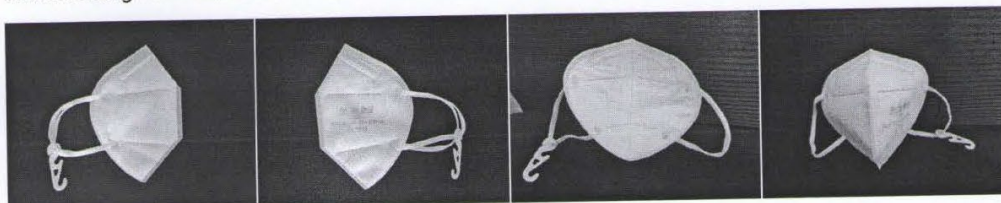

The article identified in (4) above is in conformance with the relevant Union Harmonization Legislation Regulation (EU) 2016/425.

References to the relevant harmonized standards used, including the date of the standard, or references to the other technical specifications, including the date of the specification, in relation to which conformity is declared:

| No. | Harmonized standard name |
|-----|--------------------------|
| 1 | EN 149:2001+A1:2009 |

CCQS Certification Services Limited. (NB 2834) performed the EU Type Examination (Module B) and issued the Type Examination Certificate Number:

| No. | EU Type Examination (Module B) Certificate Number |
|-----|---|
| 1 | CE-PC-200508-351-01-9A |

Product Category:

- This product is Category II.
- This product is Category III and is subject to Module C2 internal production control plus supervised product checks at random intervals and is under the surveillance of CCQS Certification Services Limited. (NB 2834)
- This product is Category III and is subject to Module D Conformity to type based on quality assurance of the production process and is under the surveillance of CCQS Certification Services Limited. (NB 2834)

Export Director Signature: S. Guangqian Date: 2020/8/8 Company stamp and/or legal signature:

